

# ***OPERATING MANUAL***

## **240 VOLT ELECTRONIC LOAD MODULE Agilent Model 60503B**



**FOR MODULES WITH SERIAL NUMBERS:  
3119A-00101 AND ABOVE**



**Agilent Technologies**

**Agilent Part No. 60503-90007  
Microfiche No. 60503-90008**

**Printed in U.S.A.  
June, 1991**

## DECLARATION OF CONFORMITY

according to ISO/IEC Guide 22 and EN 45014

**Manufacturer's Name:** Agilent Technologies

**Manufacturer's Address:** New Jersey Division  
140 Green Pond Road  
Rockaway, NJ 07866 U.S.A.

declares that the product

**Product Name:** Load mainframe and modules

**Model Number(s):** Agilent 6050A, 6051A mainframes with modules  
Agilent 60501A/B, 60502A/B, 60503A/B, 60504A/B, 60507A/B

conform(s) to the following Product Specifications:

**Safety:** IEC 348:1978 / HD401 S1:1981<sup>1</sup>

**EMC:** CISPR 11:1990 / EN 55011:1991 - Group 1, Class B  
IEC 801-2:1991 / EN 50082-1:1992 - 4kV CD, 8 kV AD  
IEC 801-3:1984 / EN 50082-1:1992 - 3 V/m  
IEC 801-4:1988 / EN 50082-1:1992 - 0.5 kV Sig. Lines, 1 kV  
Power Lines


### Supplementary Information:

The product herewith complies with the requirements of the Low Voltage Directive 73/23/EEC and the EMC Directive 89/336/EEC and carries the CE-marking accordingly.

Note 1: The product family was introduced prior to 12/93

New Jersey  
Location

January 1997  
Date



Bruce Krueger / Quality Manager

European Contact: Your local Agilent Technologies Sales and Service Office or Agilent Technologies GmbH,  
Department TRE, Herrenberger Strasse 130, D-71034 Boeblingen (FAX:+49-7031-14-3143)

# 240-Volt Module

---

## About This Manual

This manual provides information for the Agilent 60503B 250-Watt Electronic Load Module. It is designed as a supplement to the Agilent 6050A/6051A Multiple Input Mainframe Electronic Load Operating Manual (part number 06050-90001). Four tables provide the following module-specific information:

Table 60503-1 lists both the specifications and supplemental characteristics of the module. Specifications indicate warranted performance in the  $25\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$  region of the total temperature range (0 to  $55\text{ }^{\circ}\text{C}$ ). Supplemental characteristics indicate non-warranted, typical performance and are intended to provide additional information by describing performance that has been determined by design or type testing.

Table 60503-2 lists the ranges that can be programmed in constant current, constant resistance, and constant voltage modes. It shows the maximum and minimum programming values for each range. Refer to this table when programming the module locally as described in Chapter 4, or remotely as described in Chapter 5 of the operating manual.

Table 60503-3 gives the factory default values of the module. Unless you have saved your own wake-up settings, the module will be set to the factory default values whenever power is applied. See Chapter 4 in the operating manual.

Table 60503-4 provides calibration information for the module. This information is needed to perform the annual calibration procedure described in Chapter 6 of the operating manual.

---

## Module Installation and Operation

Except for the module-specific information in this manual, all installation, operation, and calibration instructions are given in the Mainframe Operating Manual. The Agilent Electronic Load Family Programming Reference Manual (part number 06060-90005) contains complete programming details that apply to all Electronic Load models.

---

**Note:** The following information in Chapter 2 of the Mainframe Operating Manual does not apply to electronic load modules with the serial numbers listed on the title page of this manual: The section titled "Extended Power Operation", and the section titled "Extended Power Limit". Also for these modules, change the 3-second delay referred to under "Nominal Power Limit" to 50 milliseconds.

---

---

## Items Supplied

In addition to this manual, a 10-pin connector plug is also shipped with your Electronic Load module. Refer to Chapter 3 in the operating manual for more information.

**Table 60503-1. Specification and Supplemental Characteristics**


**SPECIFICATIONS**

**DC Input Rating:**


**Current:** 0 to 10 A

**Voltage:** 3 V to 240 V (minimum dc operation from 0 to 2 V for 0 to 10 A)

**Power:** 250 W at 40 °C (derated to 187 W at 55 °C)

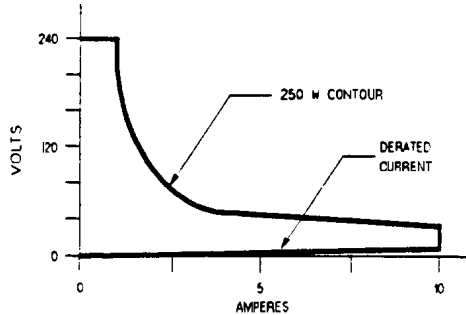

**A. OPERATING CHARACTERISTICS**

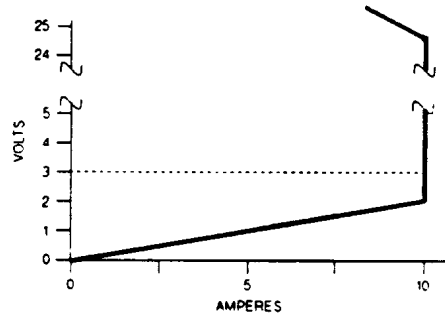

**B. DERATED CURRENT DETAIL**

**Constant Current Mode:**

**Ranges:** 0 to 1 A; and 0 to 10 A  
**Accuracy:** (after 30 second wait):  $\pm 0.15\% \pm 10$  mA (both ranges)  
**Resolution:** 0.26 mA (1 A range); 2.6 mA (10 A range)  
**Regulation:** 8 mA (both ranges)  
**Temperature Coefficient:** 150 ppm/°C  $\pm$  1 mA/°C (both ranges)

**Constant Resistance Mode:**

**Ranges:** 0.20 to 24  $\Omega$ ; 24  $\Omega$  to 10 k $\Omega$ ; and 240  $\Omega$  to 50 k $\Omega$   
**Accuracy:**  $\pm 0.8\% \pm 200$  m $\Omega$  with  $\geq 1$  A at input (24  $\Omega$  range);  
 $\pm 0.3\% \pm 0.3$  mS with  $\geq 24$  V at input (10 k and 50 k $\Omega$  ranges)  
**Resolution:** 6 m $\Omega$  (24  $\Omega$  range); 0.011 mS (10 k $\Omega$  range); 0.001 mS (50 k $\Omega$  range)  
**Regulation:** 10 mV with remote sensing (24  $\Omega$  range); 8 mA (10 k and 50 k $\Omega$  ranges)  
**Temperature Coefficient:** 800 ppm/°C  $\pm$  10 m $\Omega$ /°C (24  $\Omega$  range);  
300ppm/°C  $\pm$  0.03 mS/°C (10 k and 50 k $\Omega$  ranges)

**Constant Voltage Mode:**

**Range:** 0 to 240 V  
**Accuracy:**  $\pm 0.12\% \pm 120$  mV  
**Resolution:** 64 mV  
**Regulation:** 10 mV (remote sense); 40 mV (local sense)  
**Temperature Coefficient:** 120 ppm/°C  $\pm$  10 mV/°C

**Table 60503-1 Specifications and Supplemental Characteristics (continued)**

**Transient Operation:**

**Continuous Mode**

<b>Frequency Range:</b>	0.25 Hz to 10 kHz
<b>Frequency Resolution:</b>	4%
<b>Frequency Accuracy:</b>	3%
<b>Duty Cycle Range:</b>	3% to 97% (0.25 Hz to 1 kHz); 6% to 94% (1 kHz to 10 kHz)
<b>Duty Cycle Resolution:</b>	4%
<b>Duty Cycle Accuracy:</b>	6% of setting $\pm$ 2%

**Pulsed Mode**

<b>Pulse Width:</b>	50 $\mu$ s $\pm$ 3% minimum; 4 s $\pm$ 3% maximum
---------------------	---

**Transient Current Level (0 to 1 A and 0 to 10 A ranges):**

<b>Resolution:</b>	4 mA (1 A range); 43 mA (10 A range)
<b>Accuracy:</b>	$\pm$ 0.18% $\pm$ 13 mA (1 A range); $\pm$ 0.18% $\pm$ 50 mA (10 A range)
<b>Temperature Coefficient:</b>	180 ppm/ $^{\circ}$ C $\pm$ 1.2 mA/ $^{\circ}$ C

**Transient Resistance Level (0.20 to 24  $\Omega$ , 24  $\Omega$  to 10 k $\Omega$ , and 240  $\Omega$  to 50 k $\Omega$  ranges):**

<b>Resolution:</b>	100 m $\Omega$ (24 $\Omega$ range); 0.18 mS (10 k $\Omega$ range); 0.018 mS (50 k $\Omega$ range)
<b>Accuracy:</b>	$\pm$ 0.8% + 200 m $\Omega$ with $\geq$ 1 A at input (24 $\Omega$ range) $\pm$ 0.3% + 0.5 mS with $\geq$ 24 V at input (10 k $\Omega$ range) $\pm$ 0.3% + 0.4 mS with $\geq$ 24 V at input (50 k $\Omega$ range)

**Transient Voltage Level (0 to 240 V):**

<b>Resolution:</b>	1.0 V
<b>Accuracy:</b>	$\pm$ 0.15% $\pm$ 1.1 V
<b>Temperature Coefficient:</b>	120 ppm/ $^{\circ}$ C $\pm$ 10 mV/ $^{\circ}$ C

**Current Readback:**

<b>Resolution:</b>	2.7 mA (via GPIB); 10 mA (front panel)
<b>Accuracy:</b>	(after 30 minute wait): $\pm$ 0.12% $\pm$ 10 mA
<b>Temperature Coefficient:</b>	100 ppm/ $^{\circ}$ C $\pm$ 1 mA/ $^{\circ}$ C

**Voltage Readback:**

<b>Resolution:</b>	67 mV (via GPIB); 100 mV (front panel)
<b>Accuracy:</b>	$\pm$ 0.1% $\pm$ 150 mV
<b>Temperature Coefficient:</b>	100 ppm/ $^{\circ}$ C $\pm$ 8 mV/ $^{\circ}$ C
<b>Maximum Readback Capability:</b>	260 V (typical)

**Power Readback:**

<b>Accuracy:</b>	$\pm$ 0.2% $\pm$ 3 W
------------------	----------------------

**Table 60503-1 Specifications and Supplemental Characteristics (continued)**

**External Analog Programming 0 to 10 V (dc or ac):**

<b>Bandwidth:</b>	10 kHz (3 db frequency)
<b>Accuracy:</b>	$\pm 3\% \pm 10$ mA (0 to 1 A range) $\pm 3\% \pm 20$ mA (0 to 10 A range) $\pm 0.5\% \pm 150$ mV (0 to 240 V range)
<b>Temperature Coefficient:</b>	150 ppm/ $^{\circ}$ C $\pm 1$ mA/ $^{\circ}$ C (current ranges) 120 ppm/ $^{\circ}$ C $\pm 10$ mV/ $^{\circ}$ C (voltage range)

**External Current Monitor (0 to 10 V):**

<b>Accuracy:</b>	$\pm 3\% \pm 10$ mA (referenced to analog common)
<b>Temperature Coefficient:</b>	100 ppm/ $^{\circ}$ C $\pm 1$ mA/ $^{\circ}$ C

**External Voltage Monitor (0 to 10 V):**

<b>Accuracy:</b>	$\pm 0.4\% \pm 240$ mV (referenced to analog common)
<b>Temperature Coefficient:</b>	70 ppm/ $^{\circ}$ C $\pm 1.2$ mV/ $^{\circ}$ C

**Remote Sensing:** 5 Vdc maximum between sense and input binding posts

**Maximum Input Levels:**

<b>Current:</b>	10.2 A (programmable to lower limits)
<b>Voltage:</b>	250 V

**Minimum Operating Voltage:** 2 V (derated to 0 V at 0 A)

**PARD (20 Hz to 10 MHz noise):**

<b>Current:</b>	1 mA rms/10 mA p-p
<b>Voltage:</b>	6 mV rms

**DC Isolation Voltage:**  $\pm 240$  Vdc between + or - input binding post and chassis ground

**Digital Inputs:**

<b>V<sub>lo</sub>:</b>	0.9 V maximum at <b>I<sub>lo</sub></b> = -1 mA
<b>V<sub>hi</sub>:</b>	3.15 V minimum (pull-up resistor on input)

**Digital Outputs:**

<b>V<sub>lo</sub>:</b>	0.72 V maximum at <b>I<sub>lo</sub></b> = 1 mA
<b>V<sub>hi</sub>:</b>	4.4 V minimum at <b>I<sub>lo</sub></b> = 20 $\mu$ A

**SUPPLEMENTAL CHARACTERISTICS**

**Programmable Slew Rate** (For any given input transition, the time required will be either the total slew time or a minimum transition time, whichever is longer. The minimum transition time increases when operating with input currents under 0.2 A and decreases with input currents over 2 A. The following are typical values;  $\pm 25\%$  tolerance):

**Table 60503-1 Specifications and Supplemental Characteristics (continued)**

**Current Slew Rate:\***

Rate #	10 A Range Step	1 A Range Step	Transition Time
1	0.17 A/ms	17 A/s	8.0 ms
2	0.42 A/ms	42 A/s	3.2 ms
3	0.83 A/ms	83 A/s	1.6 ms
4	1.7 A/ms	0.17 A/ms	800 $\mu$ s
5	4.2 A/ms	0.42 A/ms	320 $\mu$ s
6	8.3 A/ms	0.83 A/ms	160 $\mu$ s
7	17 A/ms	1.7 A/ms	80 $\mu$ s
8	42 A/ms	4.2 A/ms	32 $\mu$ s
9	83 A/ms	8.3 A/ms	20 $\mu$ s
10	0.17 A/ $\mu$ s	17 A/ms	20 $\mu$ s
11	0.42 A/ $\mu$ s	42 A/ms	16 $\mu$ s
12	0.83 A/ $\mu$ s	83 A/ms	16 $\mu$ s

\*AC performance specified from 3 to 240 V.

**Voltage Slew Rate:**

Rate #	Voltage Range Step	Transition Time*
1	4 V/ms	8.0 ms
2	10 V/ms	3.2 ms
3	20 V/ms	1.6 ms
4	40 V/ms	800 $\mu$ s
5	100 V/ms	320 $\mu$ s
6	200 V/ms	160 $\mu$ s
7	0.4 V/ $\mu$ s	100 $\mu$ s
8	1 V/ $\mu$ s	100 $\mu$ s
9	2 V/ $\mu$ s	100 $\mu$ s

\*Transition time based on low capacitance current source.

**Resistance Slew Rate** (24  $\Omega$  range): Uses the value programmed for voltage slew rate.

**Resistance Slew Rate** (10 k and 50 k $\Omega$  ranges): Uses the value programmed for current slew rate.

**Transient Current Overshoot (When programmed from 0A):**

Range	Transient Current Level	Current Slew Rate	Overshoot*
10 A	2-10 A	All slew rates	0
	0.5 A	0.17 A/ $\mu$ s to 0.83 A/ $\mu$ s	5%
	0.5 A	0.17 A/ms to 42 A/ms	0
	1 A	0.83 A/ $\mu$ s	1%
	1 A	0.17 A/ms to 0.17 A/ $\mu$ s	0
1 A	0.5 A	8.3 A/ms	4%
	0.5 A	0.17 A/s and 0.17 A/ms	0
	1 A	All slew rates	0

\*All overshoot values assume a total inductance of 1 $\mu$ H, or less, in the load leads connected to the D.U.T.

**Table 60503-1 Specifications and Supplemental Characteristics (continued)**

**Source Turn-On Current Overshoot:** Less than 5% of final value (in CC and CR modes when connected to power supplies with voltage rise times of greater than 500µs).

**Programmable Short Circuit:** 0.20 Ω (0.10 Ω typical)

**Programmable Open Circuit:** 80 kΩ (typical)

**Drift Stability** (over an 8 hour interval):

**Current:** ±0.03% ±1.5 mA  
**Voltage:** ±0.01% ±20 mV

**Reverse Current Capacity:** 20 A when unit is on; 10 A when unit is off

**Weight:** 3.2 kg (7 lbs.)

**Table 60503-2. Programming Ranges**

Function	Front Panel Key	Front Panel Display	HPSL Command (Short Form)	Range of Values
<b>Constant Current</b>				
Set Range	<b>Range</b>	C:RNG value	"CURR:RANG value"	≥ 0 and ≤ 1 A > 1 A and ≤ 10 A
Low Range				
High Range				
Set Main Level	<b>CURR</b>	CURR value	"CURR value"	0 to 1 A 0 to 10 A
Low Range				
High Range				
Set Slew Rate	(shift) <b>Slew</b>	C:SLW value	"CURR:SLEW value"	0.000007 to .083 (A/µs) 0.00017 to 0.83 (A/µs)
Low Range				
High Range				
Set Transient Level	<b>Tran Level</b>	C:Tlv value	"CURR:TLEV value"	same as main level
*Set Triggered Level			"CURR:TRIG value"	same as main level
<b>Constant Resistance</b>				
Set Range	<b>Range</b>	R:RNG value	"RES:RANG value"	≥ 0 and ≤ 24 Ω > 24 Ω and ≤ 24 kΩ >24 kΩ and ≤ 24 kΩ
Low Range				
Middle Range				
High Range				
Set Main Level	<b>RES</b>	RES value	"RES value"	0 to 24 Ω 24 Ω to 24 kΩ 240 Ω to 240 kΩ
Low Range				
Middle Range				
High Range				
Set Slew Rate	(shift) <b>Slew</b>	V:SLW value C:SLW value	"VOLT:SLEW value" "CURR:SLEW value"	same as voltage slew same as current slew
Low Range				
Middle/High Range				
Set Transient Level	<b>Tran Level</b>	R:Tlv value	"RES:TLEV value"	same as main level
*Set Triggered Level			"RES:TRIG value"	same as main level
<b>Constant Voltage</b>				
Set Main Level	<b>VOLT</b>	VOLT value	"VOLT value"	0 to 240 V
Set Slew Rate	(shift) <b>Slew</b>	V:SLW value	"VOLT:SLEW value"	0.004 to 2 (V/µs)
Set Transient Level	<b>Tran Level</b>	V:Tlv value	"VOLT:TLEV value"	same as main level
*Set Triggered Level			"VOLT:TRIG value"	same as main level



**Table 60503-2. Programming Ranges (continued)**

Function	Front Panel Key	Front Panel Display	HPSL Command (Short Form)	Range of Values
<b>Transient Operation</b> Set Frequency Set Duty Cycle  *Set Pulse Width	<b>FREQ</b>  (shift) <b>Dcycle</b>	FREQ value DCYCLE value	"TRAN:FREQ value" "TRAN:DCYC value"  "TRAN:TWID value"	0.25 Hz to 10 kHz 3-97% (0.25 Hz-1 kHz) 6-94% (1 kHz-10 kHz) 0.00005 to 4 s
<b>Trigger Operation</b> *Set Trigger Period			"TRIG:TIM value"	0.000008 to 4 s
<b>Current Protection</b> *Set Current Level *Set Delay Time			"CURR:PROT value" "CURR:PROT:DEL value"	0 to 10.2 A 0 to 60 s
*Can only be programmed remotely via the GPIB.				

**Table 60503-3. Factory Default Settings**

Function	Settings	Function	Setting
CURR level	0 A	Mode (CC, CR, CV)	CC
CURR transient level	0 A	Input (on/off)	on
*CURR slew rate	0.17 A/μs	Short (on/off)	off
CURR range	10 A	Transient operation (on/off)	off
*CURR protection (on/off)	off	***TRAN mode	continuous
**CURR protection level	10.2 A	(continuous, pulse, toggle)	
**CURR protection delay	15 s	TRAN frequency	1 kHz
RES level	50 kΩ	TRAN duty cycle	50%
RES transient level	50 kΩ	**TRAN pulse width	0.5 ms
RES range	50 kΩ	**TRIG source	hold
VOLT level	240 V	(bus, external, hold, timer, line)	
VOLT transient level	240 V	**TRIG period	0.001 s
VOLT slew rate	2 V/μs	**PORT0 output (on/off)	off (logic 0)
		**CAL mode (on/off)	off
<p>The *RST command resets the CURR slew rate to 0.83 A/μ, not to the factory default.</p> <p>**Can only be programmed remotely via the GPIB.</p> <p>***Continuous transient mode is the only mode available at the front panel. Pulsed, toggled, and continuous modes can all be programmed remotely via the GPIB.</p>			

**Table 60503-4. Calibration Information**

<b>Ranges and Calibration Points</b>	<b>Variables</b>	<b>Variables Value</b>	<b>Power Supply Settings</b>	<b>Current Shunt</b>
High Current Range High Current Offset	Hi_curr_rng Hi_curr_offset	10 0.0048	25 V/10.5 A	15 A
Low Current Range Low Current Offset	Lo_curr_rng Lo_curr_offset	1 0.0032	25 V/2 A	15 A
Voltage Range Voltage Hi point Voltage Lo point	N/A Volt_hipt Volt_lopt	N/A 240 2	246 V/0.6 A	N/A
Low Resistance Range Low Resistance Hi point Low Resistance Lo point	Lo_res_rng Lo_res_hipt Lo_res_lopt	24 23.9 0.88	60 V/1.82 A	15 A
Middle Resistance Range Middle Resistance Hi point Middle Resistance Lo point	Mid_res_rng Mid_res_hipt Mid_res_lopt	240 500 24	43.6 V/4 A	15 A
High Resistance Range High Resistance Hi point High Resistance Lo point	Hi_res_rng Hi_res_hipt Hi_res_lopt	24020 2000 240	240 V/2 A	15 A

## Agilent Sales and Support Office

For more information about Agilent Technologies test and measurement products, applications, services, and for a current sales office listing, visit our web site: <http://www.agilent.com/find/tmdir>

You can also contact one of the following centers and ask for a test and measurement sales representative.

### United States:

Agilent Technologies  
Test and Measurement Call Center  
P.O. Box 4026  
Englewood, CO 80155-4026  
(tel) 1 800 452 4844

### Latin America:

Agilent Technologies  
Latin American Region Headquarters  
5200 Blue Lagoon Drive, Suite #950  
Miami, Florida 33126  
U.S.A.  
(tel) (305) 267 4245  
(fax) (305) 267 4286

### Canada:

Agilent Technologies Canada Inc.  
5150 Spectrum Way  
Mississauga, Ontario  
L4W 5G1  
(tel) 1 877 894 4414

### Australia/New Zealand:

Agilent Technologies Australia Pty Ltd  
347 Burwood Highway  
Forest Hill, Victoria 3131  
(tel) 1-800 629 485 (Australia)  
(fax) (61 3) 9272 0749  
(tel) 0 800 738 378 (New Zealand)  
(fax) (64 4) 802 6881

### Europe:

Agilent Technologies  
Test & Measurement European Marketing Organisation  
P.O. Box 999  
1180 AZ Amstelveen  
The Netherlands  
(tel) (31 20) 547 9999

### Asia Pacific:

Agilent Technologies  
24/F, Cityplaza One, 1111 King's Road,  
Taikoo Shing, Hong Kong  
tel: (852)-3197-7777  
fax: (852)-2506-9284

### Japan:

Agilent Technologies Japan Ltd.  
Measurement Assistance Center  
9-1, Takakura-Cho, Hachioji-Shi,  
Tokyo 192-8510, Japan  
(tel) (81) 426 56 7832  
(fax) (81) 426 56 7840  
Technical data is subject to change.