


# LC77

## “AUTO-Z”

# CAPACITOR – INDUCTOR ANALYZER

Operation, Application, and Maintenance Manual

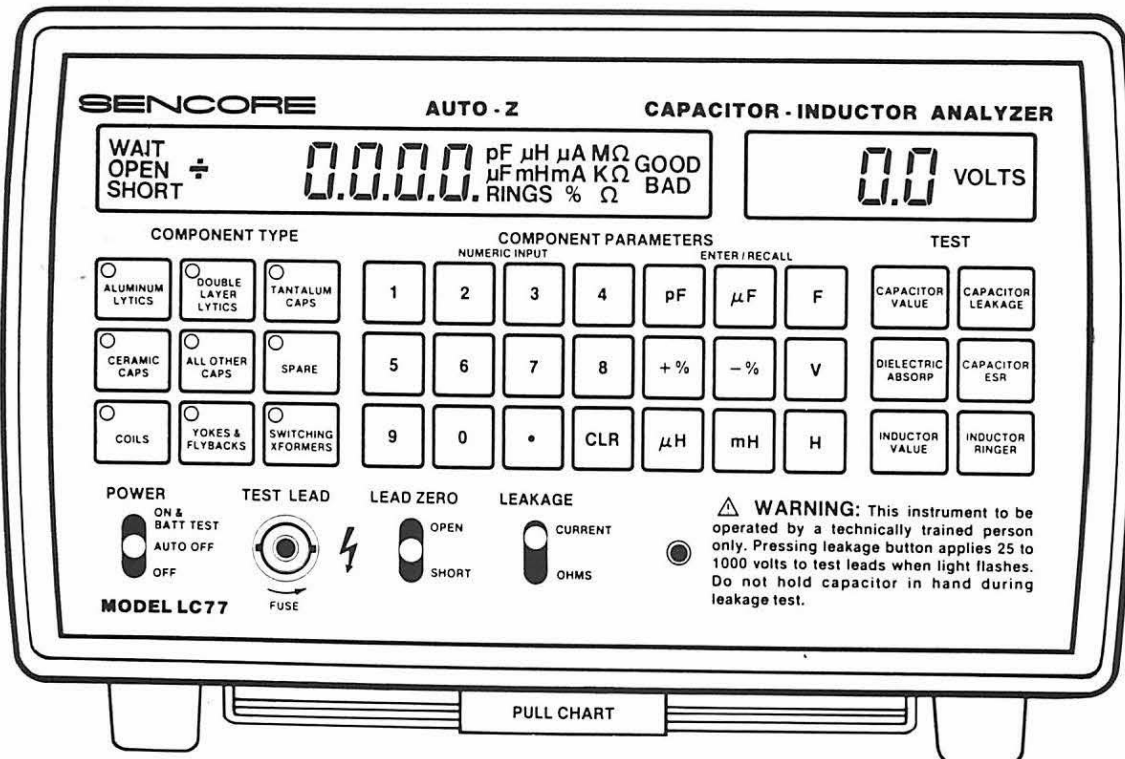

**SENCORE**  
 3200 Sencore Drive, Sioux Falls, SD 57107